


HPLC DATA SHEET

Sitagliptin, Metformin

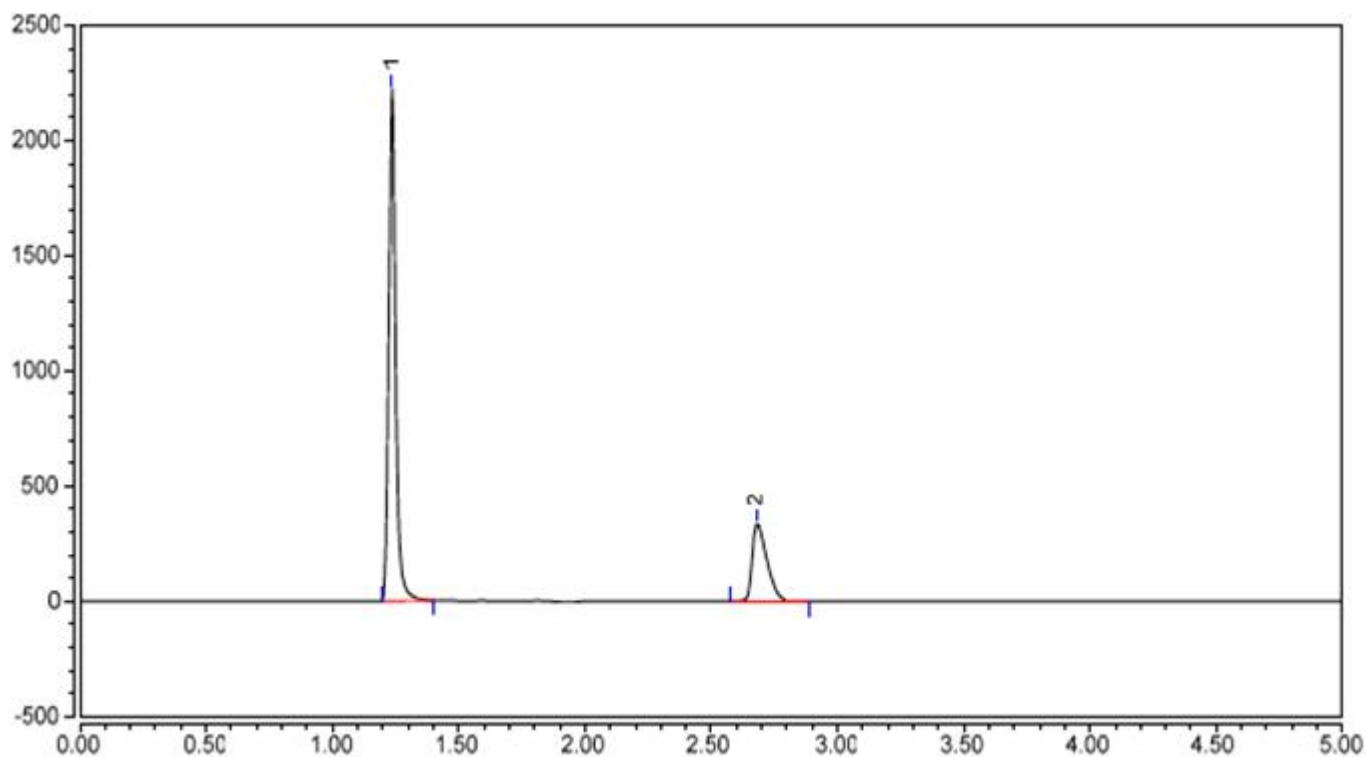

1. Metformin 2. Sitagliptin

HPLC condition

Column	INNO column C18, 5um (4.6×150mm)
Mobile Phase	Water / ACN / Phosphoric acid= 700 / 300 / 1
Flow rate	1.0 mL/min
Temperature	35℃
Detector	UV (210nm)